

Instructions for Use
BEVESPI AEROSPHERE®
(be-VES-pee AIR-oh-sfeer)
(glycopyrrolate and formoterol fumarate)
Inhalation aerosol, for oral inhalation use

Read this Instructions for Use before you start using BEVESPI AEROSPHERE and each time you get a refill. There may be new information. This information does not take the place of talking to your healthcare provider about your medical condition or treatment.

Important Information:

- **For oral inhalation use only.**
- Use BEVESPI AEROSPHERE exactly as your healthcare provider tells you to.
- If you have any questions about the use of your inhaler, ask your healthcare provider or pharmacist.

Parts of your BEVESPI AEROSPHERE inhaler (See Figure 1):

- BEVESPI AEROSPHERE comes as a canister that fits into an actuator with a dose indicator.
 - **Do not** use the BEVESPI AEROSPHERE actuator with a canister of medicine from any other inhaler.
 - **Do not** use the BEVESPI AEROSPHERE canister with an actuator from any other inhaler.

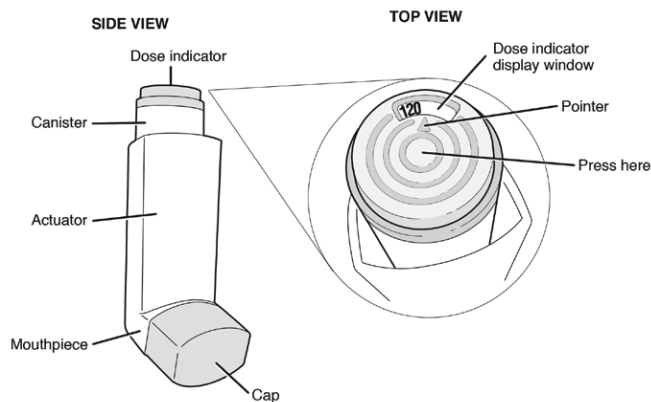


Figure 1

- BEVESPI AEROSPHERE comes with a dose indicator located on the top of the canister (See Figure 1). The dose indicator display window will show you how many puffs of medicine you have left. A puff of medicine is released each time you press the center of the dose indicator.

Before you use BEVESPI AEROSPHERE for the first time make sure that the pointer on the dose indicator is pointing to the right of the “120” inhalation mark in the dose indicator display window (See Figure 1).

- The pointer will be pointing to 120 after 10 puffs are delivered from BEVESPI AEROSPHERE. This means that there are 120 puffs of medicine left in the canister (See Figure 2a).
- The pointer will be pointing between 100 and 120 after you take 10 more puffs. This means that there are 110 puffs of medicine left in the canister (See Figure 2b).

- The pointer will be pointing to 100 after you take 10 more puffs. This means that there are 100 puffs of medicine left in the canister (See Figure 2c).



Figure 2a
120 puffs



Figure 2b
110 puffs



Figure 2c
100 puffs

- The dose indicator display window will continue to move after every 10 puffs. The number in the dose indicator display window will continue to change after every 20 puffs.



Figure 2d

- The color in the dose indicator display window will change to red, as shown in the shaded area, when there are only 20 puffs of medicine left in your inhaler (See Figure 2d).

Preparing your BEVESPI AEROSPHERE inhaler for use:

- BEVESPI AEROSPHERE should be at room temperature before you use it.
- Your BEVESPI AEROSPHERE inhaler comes in a foil pouch that contains a drying packet (desiccant).
 - Take the BEVESPI AEROSPHERE inhaler out of the foil pouch.
 - Throw away the pouch and the drying packet. Do not eat or breathe in the contents of the drying packet.

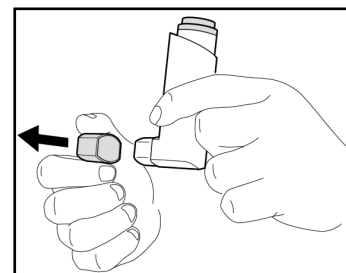


Figure 3

Priming your BEVESPI AEROSPHERE inhaler:

Before you use BEVESPI AEROSPHERE for the first time, you must prime the inhaler.

- Remove the cap from the mouthpiece (See Figure 3). Check inside the mouthpiece for objects before use.
- Hold the inhaler in the upright position away from your face and shake the inhaler well (See Figure 4).

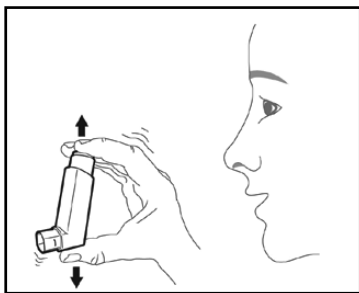


Figure 4

- Press down firmly on the center of the dose indicator until the canister stops moving in the actuator, to release a puff of medicine from the mouthpiece (See Figure 5). You may hear a soft click from the dose indicator as it counts down during use.

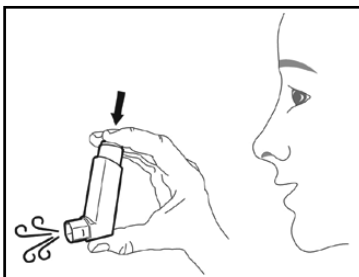


Figure 5

- Repeat the priming steps 3 more times (See Figure 4 and Figure 5). Shake the inhaler well before each priming puff.
- After priming 4 times, the dose indicator should be pointing to the right of "120" and your inhaler is now ready to use.

Using your BEVESPI AEROSPHERE inhaler:

Step 1: Remove the cap from the mouthpiece (See Figure 6).

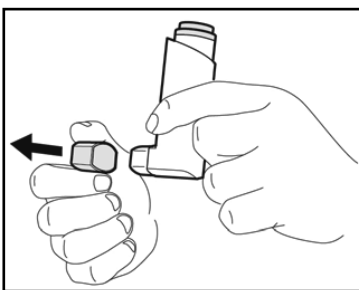


Figure 6

Step 2: Shake the inhaler well before each use (See Figure 7).

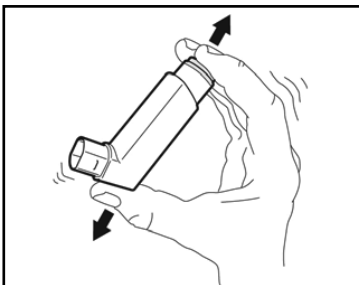


Figure 7

Step 3: Hold the inhaler with the mouthpiece pointing towards you and breathe out as fully as you comfortably can through your mouth (See Figure 8).

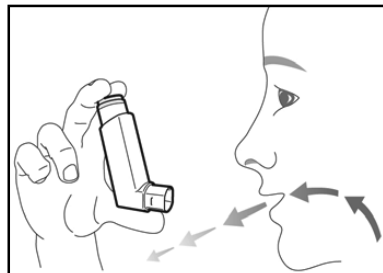


Figure 8

Step 4: Close your lips around the mouthpiece and tilt your head back, keeping your tongue below the mouthpiece (See Figure 9).

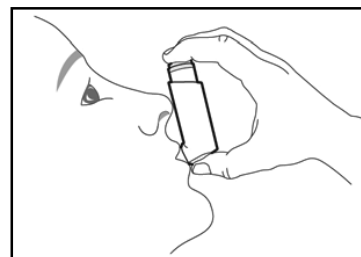


Figure 9

Step 5: While breathing in deeply and slowly, press down on the center of the dose indicator until the canister stops moving in the actuator and a puff of medicine has been released (See Figure 10). Then stop pressing the dose indicator.

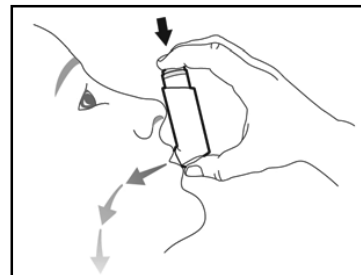


Figure 10

Step 6: When you have finished breathing in, remove the mouthpiece from your mouth. Hold your breath as long as you comfortably can, up to 10 seconds (See Figure 11).

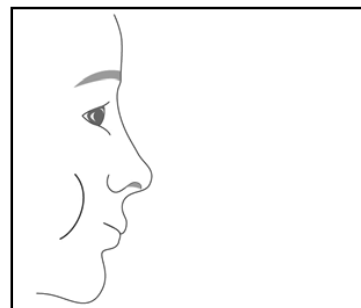


Figure 11

Step 7: Breathe out gently (See Figure 12). Repeat steps 2 through 7 to take your second puff of BEVESPI AEROSPHERE.

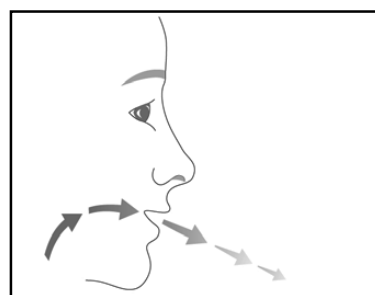


Figure 12

Step 8: Replace the cap over the mouthpiece right away after use (See Figure 13).

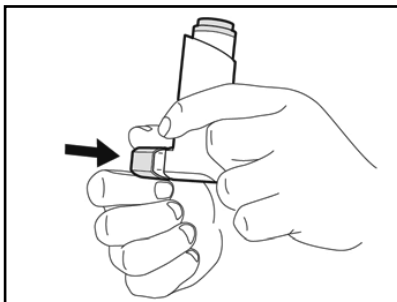


Figure 13

How to clean your BEVESPI AEROSPHERE inhaler:

Clean the inhaler 1 time each week. It is very important to keep your inhaler clean so that medicine will not build-up and block the spray through the mouthpiece (See Figure 14).

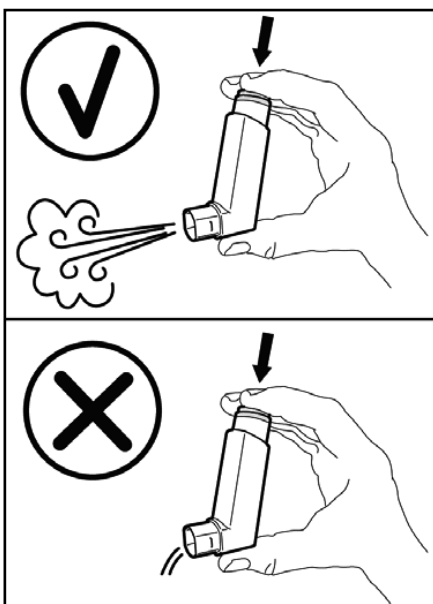


Figure 14

Step 1: Take the canister out of the actuator (See Figure 15). **Do not** clean the canister or let it get wet.

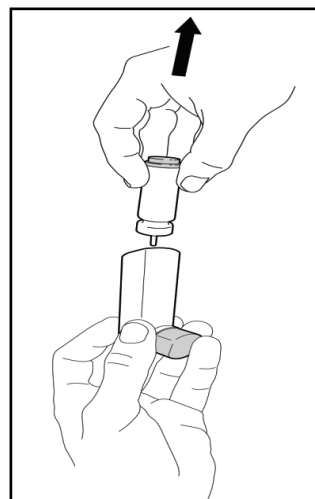


Figure 15

Step 2: Take the cap off the mouthpiece.

Step 3: Hold the actuator under the faucet and run warm water through it for about 30 seconds. Turn the actuator upside down and rinse the actuator again through the mouthpiece for about 30 seconds (See Figure 16).

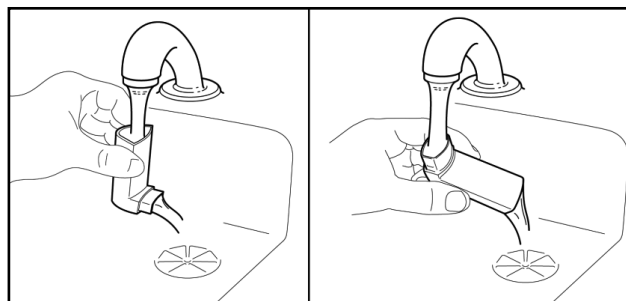


Figure 16

Step 4: Shake off as much water from the actuator as you can.

Step 5: Look into the actuator and the mouthpiece to make sure any medicine build-up has been completely washed away. If there is any build-up, repeat Steps 3 through 5 in the section “How to clean your BEVESPI AEROSPHERE inhaler”.

Step 6: Let the actuator air-dry overnight (See Figure 17). **Do not** put the canister back into the actuator if it is still wet.

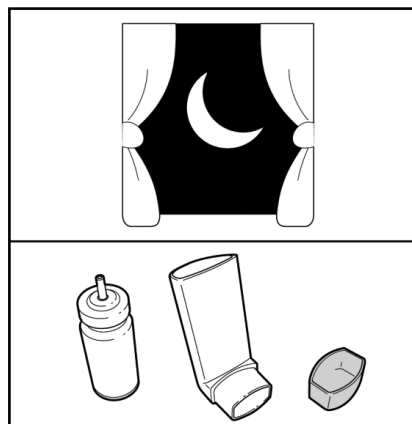


Figure 17

Step 7: When the actuator is dry, gently press the canister down in the actuator (**See Figure 18**). Do not press down too hard on the canister. This could cause a puff of medicine to be released.

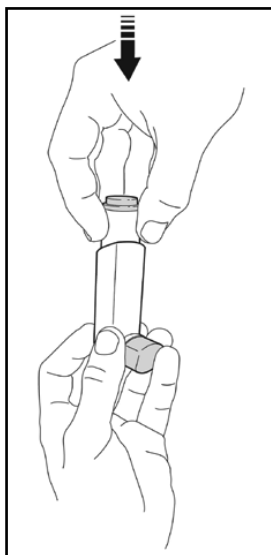


Figure 18

Step 8: Re-prime your **BEVESPI AEROSPHERE** inhaler after each cleaning. To re-prime the inhaler, shake the inhaler well and press down on the center of the dose indicator 2 times to release a total of 2 puffs into the air away from your face. Your inhaler is now ready to use.

If you do not use your BEVESPI AEROSPHERE for more than 7 days, you will need to re-prime it before use.

To re-prime the inhaler, shake the inhaler well and press down on the center of the dose indicator 2 times to release a total of 2 puffs into the air away from your face. Your inhaler is now ready to use.

BEVESPI and BEVESPI AEROSPHERE are registered trademarks of the AstraZeneca group of companies.

Distributed by: AstraZeneca Pharmaceuticals LP, Wilmington, DE 19850

©AstraZeneca 2023

This Instructions for Use has been approved by the U.S. Food and Drug Administration.

Revised: March 2023 US-74563 4/23